


UTM-DCH

Computerized Dual-column Servo Tensile Testing Machine



Contact us

Mikrosize Precision Instrument Co.,Ltd

A-4035 RuiFeng Business Expo, Wuhu City, China , 241000.

Web: www.mikrosize.com

Email: mikrosize@mikrosize.com






Feature and Application

Product Feature


- Fully computer-controlled testing machines, international speed control technology.
- International brands components, making the machine with long-term high reliability, stability, and precision, as well as smooth operation and a long lifespan.
- Used for material testing with loads below 50 KN and covers a wide range of testing functions for most products, making it an ideal mechanical testing instrument for factories, research institutes, and quality inspection agencies.
- Fully digital, closed-loop (force, deformation, displacement) control system with adaptive PID algorithms achieves fully digital closed-loop control of force and displacement, allowing automatic switching between control loops and ensuring smooth transitions without impact when switching between different modes.

Product Application

- Suitable for mechanical performance tests and analysis such as tension, compression, peel, tear, and shear; suitable for Medium-strength Metal, Sintered product, friction material, rubber, plastic, thin film, fiber and fine thread, adhesive, foam material, adhesive tape, elastomer, connector, bio-material, wood products and paper products, metal foil, wire, oil bearing, ceramics, parts and components, fastener, composite material.



Product Details



1.Limit Device


2.Force Sensor

3.Fixture

4.Emergency Stop Button

5.Power Switch

6.Leveling Feet



1.Power cord socket

2.Socket for computer connection (optional)

3.Socket for the extension meter (optional)


Product Details

Detailed Display




- This equipment adopts high-precision force value sensor to ensure the accuracy of experimental data;
- The fixture can be quickly loaded and unloaded, loosen the fixture lock nut, pull out the fixture pin, you can remove the fixture, installation is installed in the reverse order;
- This equipment can be adapted to a variety of fixtures to meet the requirements of different experiments.

- Extensometer(optional)
- Extensometer with double encoder up and down extension axial structure, with rotating device, can be quickly loaded and unloaded, clamping strength tight, smooth operation, no inertia hysteresis, rugged, accurate measurements.



Screen Interface


Panel Control

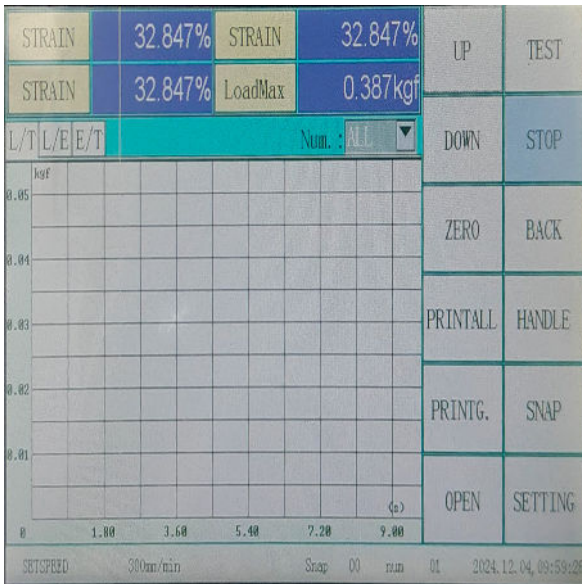

- The display screen of this machine adopts touch control method, which is easy and convenient to operate, in this interface you can:
 1. Control the lifting and lowering of the tensile strength machine and the start and stop of the experiment.
 2. Zeroing of the test data and the machine back to the position (press the "back to the button", the machine will return to the position of the most recent time to press the "zero" button moment, the process can be at any time by pressing the "stop" button) (The process can be stopped at any time by pressing the "stop button")
 3. Printing out the test results

Selecting Display Parameters

- Click on the parameter section to select the desired parameter to be displayed, and the parameters that can be selected are: Load; Stroke; Load Max; Elong; Real Speed; Test Time; P.H Time; STRESS; SIRAIN.

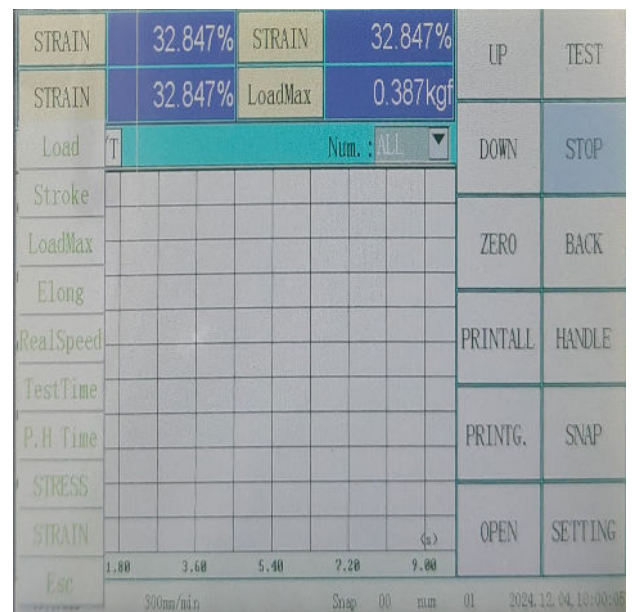


Screen Interface

Group and Plot Coordinate Selection



- When several groups of tests have been conducted, click "Num" to view the curve graph corresponding to the desired test group. The machine has three kinds of curve graphs, respectively, force value - time (L/T); force value - displacement (L/E); displacement - time (E/T), click the corresponding button to switch.

Manual Control of Speed Adjustment

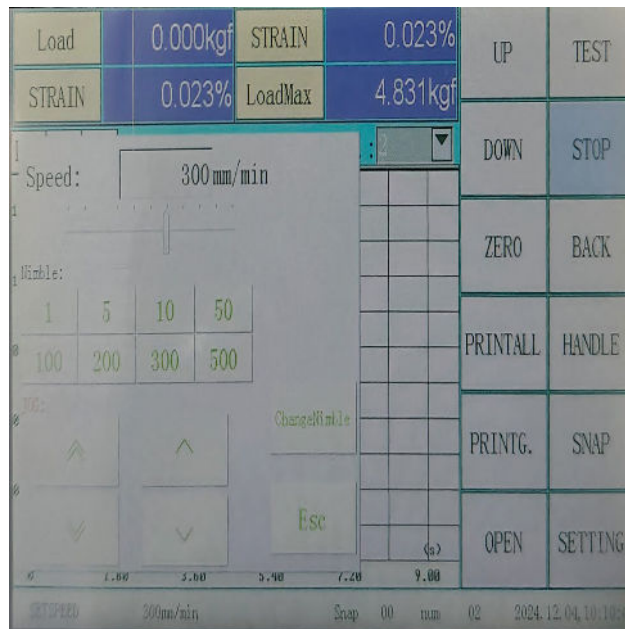

- Press the "Manual Control" button to enter this interface, you can adjust the speed of the manual control, users can directly in the "Nimble" quickly select the desired speed, you can also slide the square to adjust the speed freely.

Screen Interface

Specimen Information

1. Sample Num:	1			Sample
2. Sample Shape:	Square			Scheme
	Circular			Result
	Square			CurveSet
No.	Gauge (mm)	φ (mm)	Thickness (mm)	Unit
1	45.000	4.000	2.620	About
				CAL I.
				TEST_INF

- This interface allows the user to set the number of specimens to be tested and the shape of the specimen.


Test Methods

- The main functions of this interface are:
- 1. Set the test speed;
- 2. Select test direction, up or down;
- 3. Setting the stopping condition;
- 4. Setting of breakpoint judgment: after entering the test, when the force value reaches the set condition value, the breakpoint ratio in the shutdown condition will be judged, which is generally set as 1% of the range of the force value sensor;
- 5. Setting of conditions for the start of deformation counting: when the force value reaches the set condition value after clicking test, it will be counted as entering the test, and the general setting is 0.1%-1% of the range of the force value sensor.

1. TestSpeed:	1	mm/min	<input type="checkbox"/> Use PreSpeed	Sample	
2. Test Dir.:	DOWN		10	mm/min	Scheme
3. A. StopTest:	Break Judge		Preload:		Result
Break S.:	50	%	0	% 0.000kgf	CurveSet
					Unit
					Method
					About
4. Break Judge:	0.1	%Range			Supply1
5. Cal. Elong:	0.1	kgf			Supply2
					TEST_INF

Screen Interface


Downtime Condition

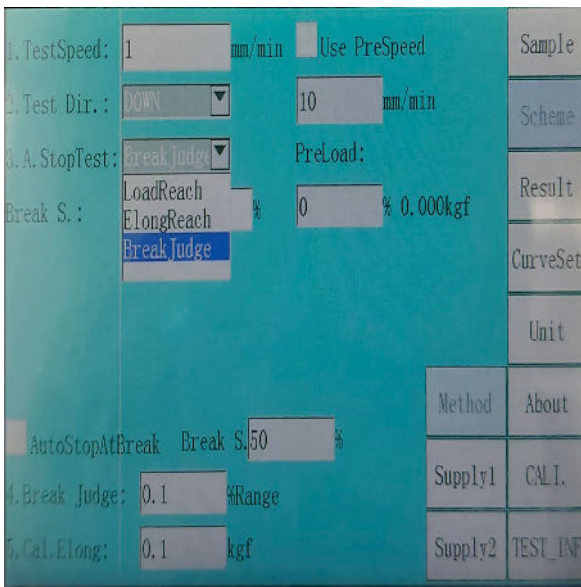


- There are three types of stopping conditions for this machine, namely:
 - “Force value reached”;
The test ends when the force value in the test reaches the set value;
 - “Displacement reached”;
The test is completed when the deformation in the test reaches the set displacement value;
 - “Breakpoint Ratio”
Generally set to 50%, set the value of the break point ratio of 50%, that is, the current force value in the test fell to 50% of the maximum force value when judged as the specimen fracture, the test is complete.

Control Parameter

- The main functions of this interface are:
 - Select the mode of the “Zero” button in the main interface of the test, with “All Zero” and “Force Zero” as options.
 - The direction of deformation, force and displacement, “reverse”, “non-reverse”, “absolute value” can be selected.
 - Select the deformation sensor, there are “displacement”, “rubber extensometer (also called large deformation)”, “metal extensometer (also called small deformation)” can be selected, the latter two for the optional accessories
 - Select the channel of force sensor




Screen Interface

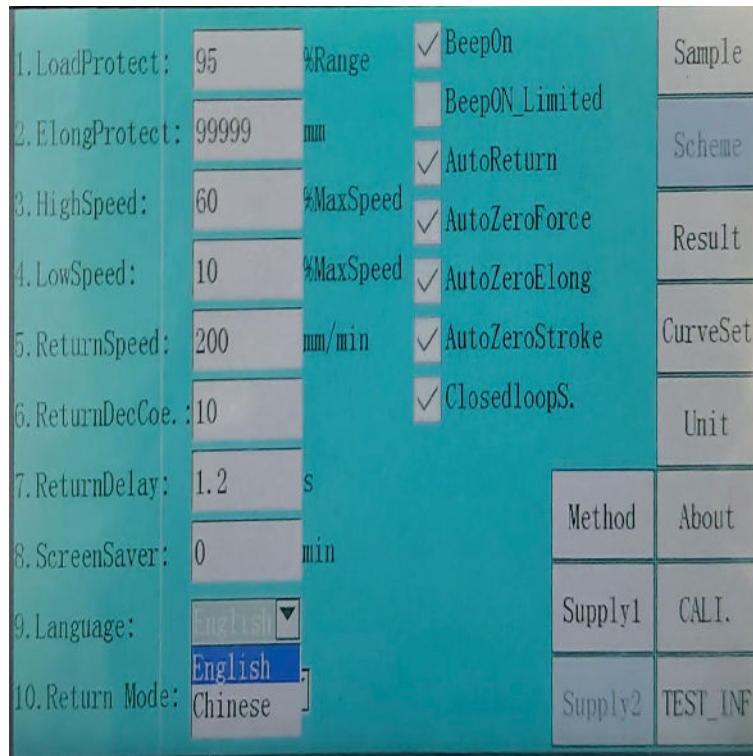

- The main functions of this interface are:
- 1. Protection setting, force value protection and deformation protection, you can set the protection parameters according to the need;
- 2. Setting the speed and waiting time of return and deceleration coefficient, the function of deceleration coefficient is: when the travel is less than the set value when returning to the position, it starts to decelerate automatically, so as to prevent overshooting of the displacement;
- 3. Set the number of digits displayed after the decimal point of the force value;
- 4. Switch the language display, "English" and "Chinese" are optional;
- 5. Select the return mode, with "displacement zero point" and "limit position" optional.
- 6. Beep when touching the screen and triggering the limit.
- 7. Automatic zeroing of displacement, force and deformation before testing, and automatic return to the position after testing is completed.


Screen Interface

Test Result Selection

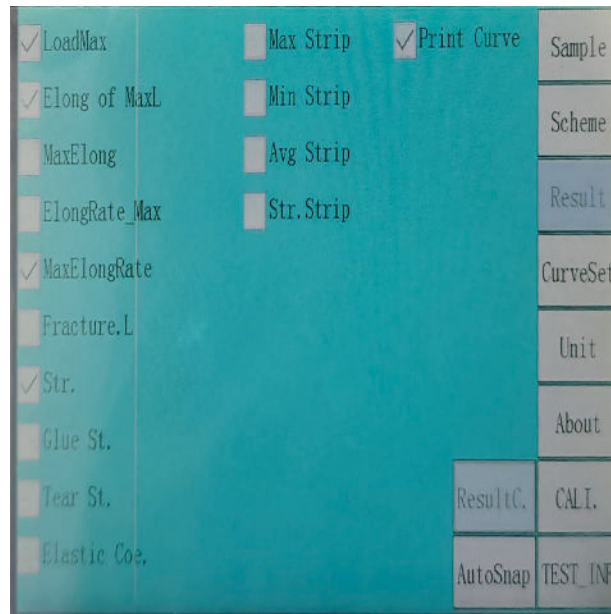

- Select the desired test results, the checked items will be displayed in the view report.


Auto Fetch Points




- Setting curve coordinates.

Screen Interface

Unit Selection

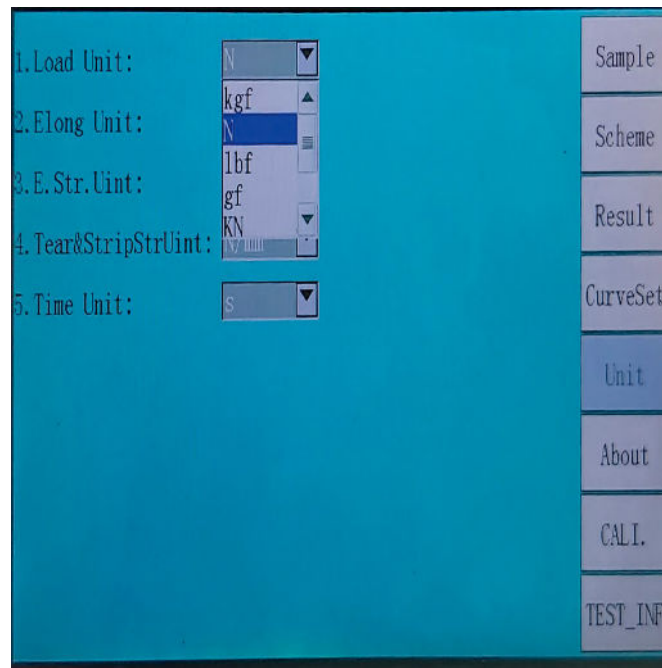


- Switching force units, "kgf", "N", "lbf", "gf", "KN", "t" are available. "KN", "t" can be selected.

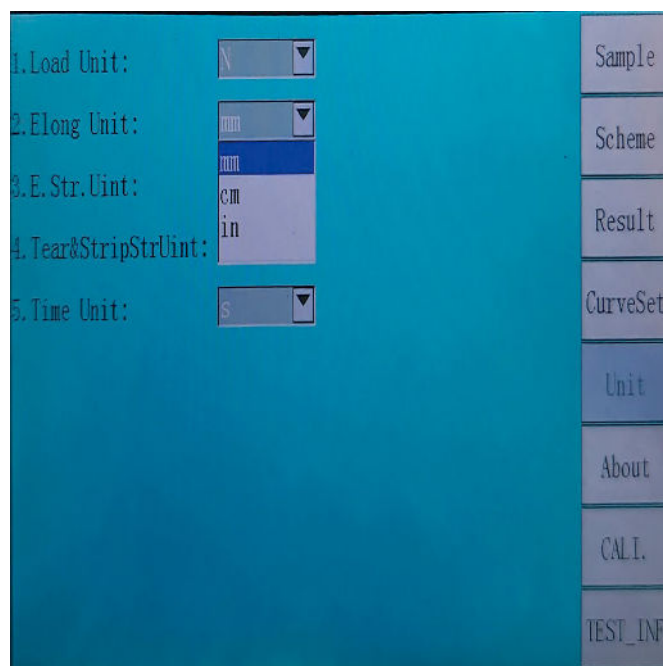


- Toggle the unit of deformation, "mm", "cm", "in" can be selected.

Screen Interface

Unit Selection

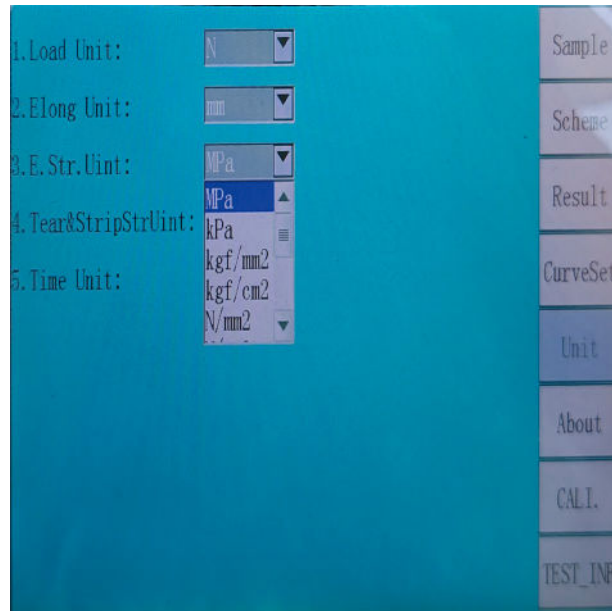


- Toggle tensile strength units with: MPa; kPa; kgf/mm²; kgf/cm²; N/mm²; N/cm²; N/m²; gf/mm²; gf/cm²; psi; lbf/in², etc.

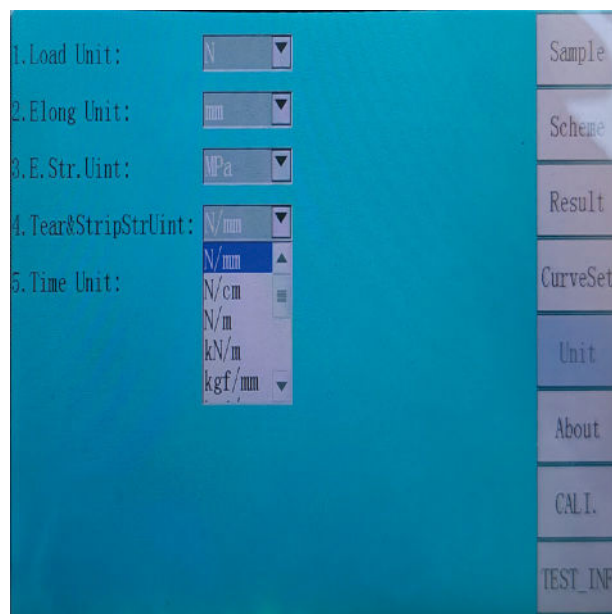

- Toggle tear peel strength units with: N/mm; N/cm; N/m; kN/m; kgf/mm; kgf/cm; kgf/m; gf/mm; gf/cm; lbf/in; klf/in, etc.


Screen Interface

Unit Selection

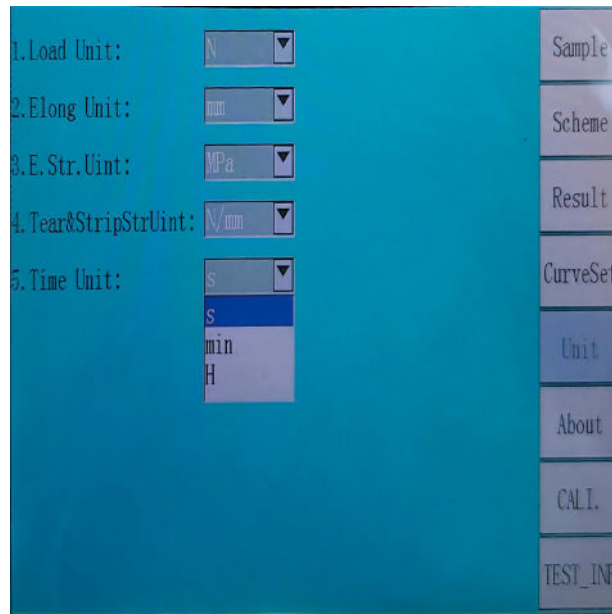

- Switch the unit of deformation, "s", "min", "H" can be selected.


Time Setting

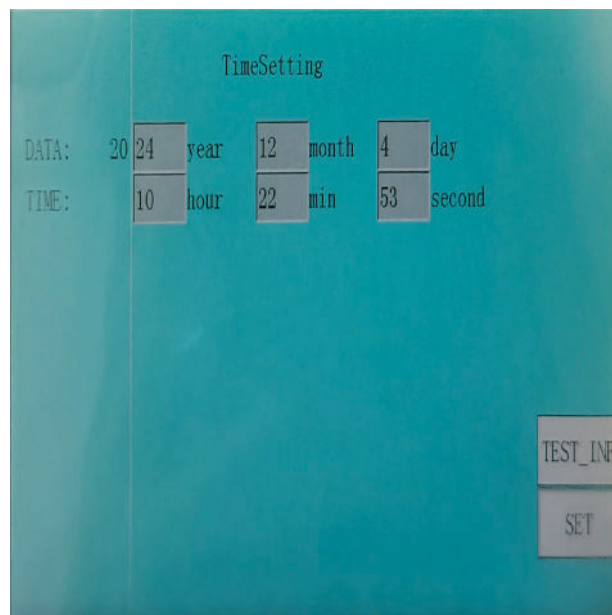

- Setting the system time.

Software Interface

Operation Interface

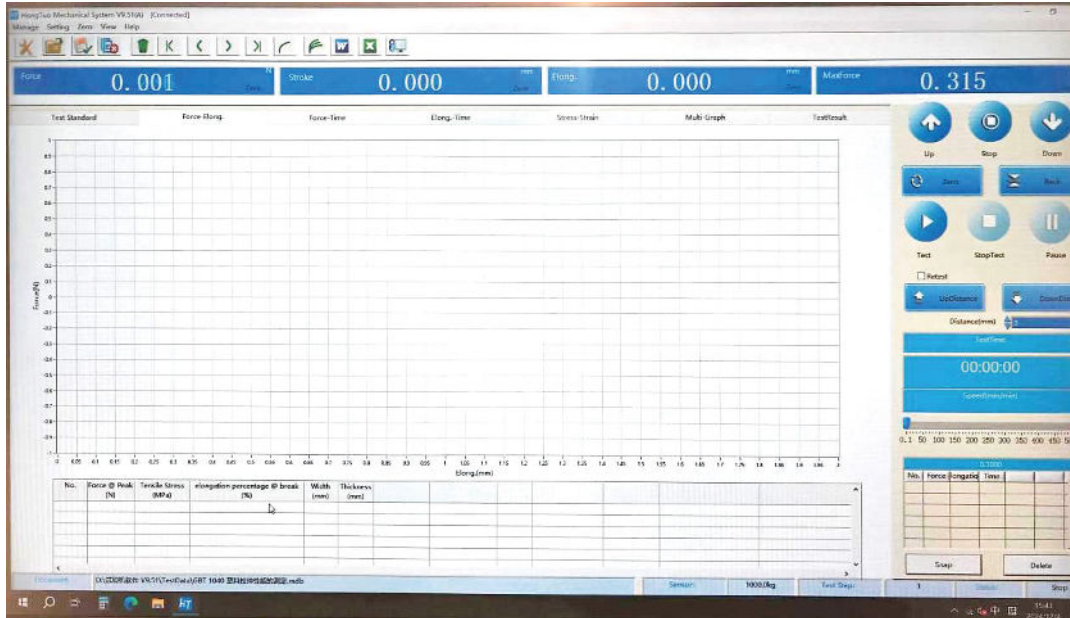

- Mainly includes standard modification, file creation, report output, curve display, test result display, image pickup point setting, instrument movement speed, and the right instrument operation button.


Test Standard Interface



- Specimen Data Interface: Specimen data viewing and editing, specimen parameter copying.

Software Interface


Test Program Interface

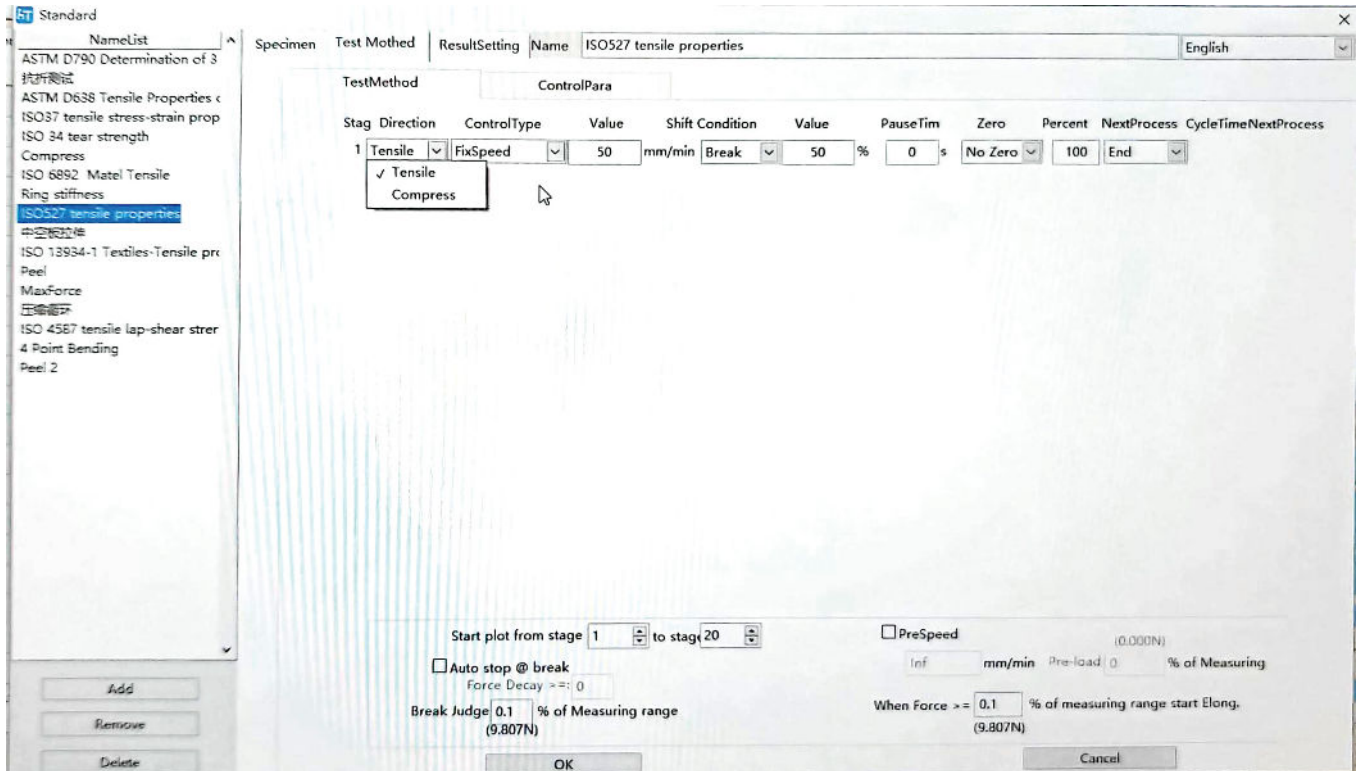

- Test Method Interface:
- 1. Control of test direction including tension and compression.
- 2. Control mode selection includes constant speed, constant deformation, constant force rate, constant force, constant stress rate, constant stress, constant strain rate, constant strain.
- 3. Setting the corresponding control values and switching conditions.
- 4. Control the condition value, pause time and control parameters.
- 5. Whether to clear when the switching condition is reached includes not clearing, force clearing, displacement clearing, deformation clearing, force and displacement clearing, force and deformation clearing, displacement and deformation clearing, and all clearing.

Software Interface


Test Program Interface

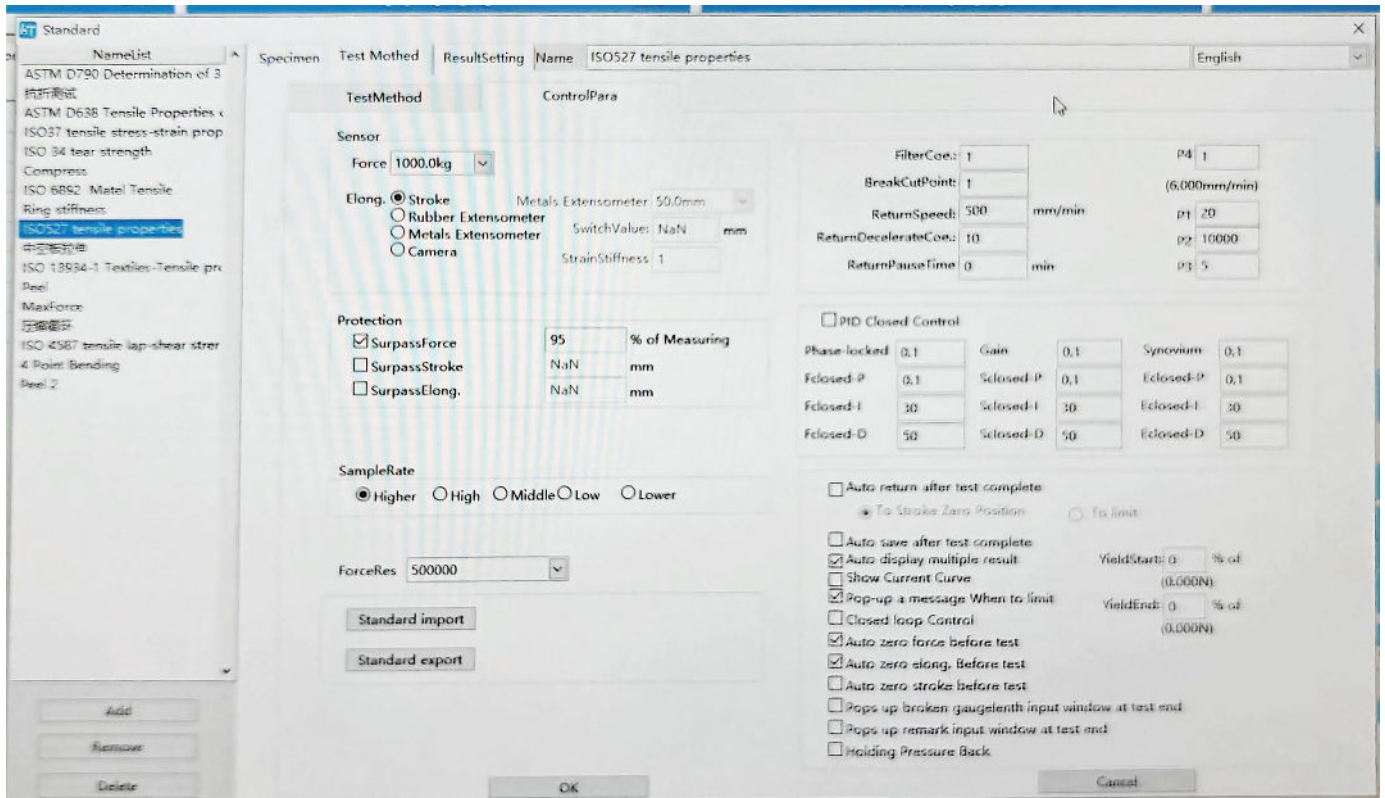


- Control Parameter Interface: Control of sensors, protection, sampling rate, power resolution, filter coefficients, break removal points, return speed, return deceleration coefficient, return wait time, etc.

Software Interface

Results Setting Screen

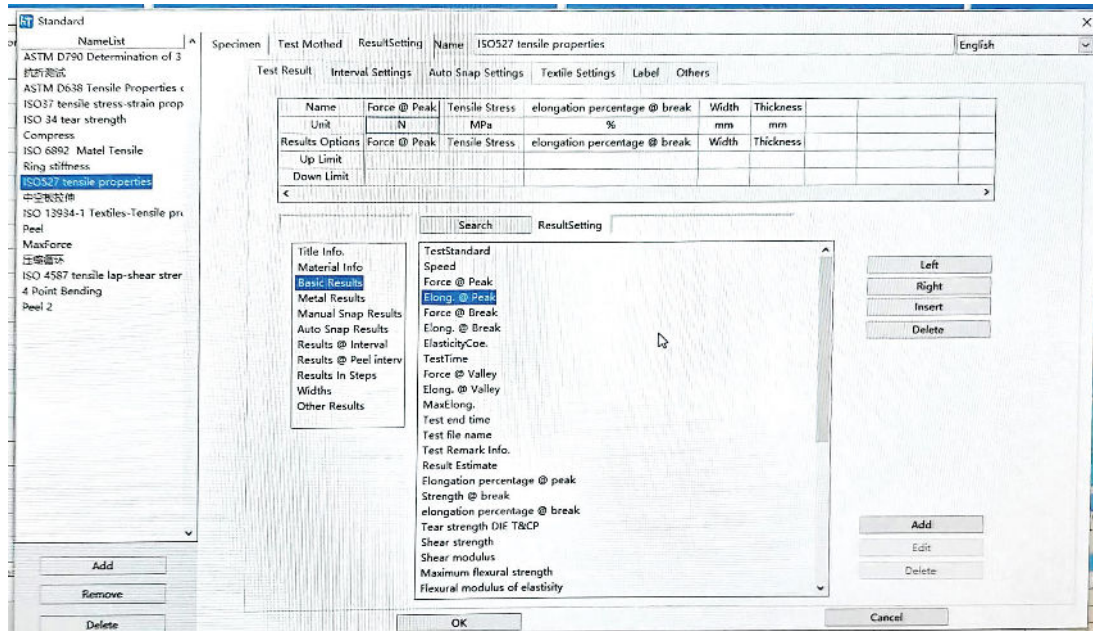


- Test results screen: Display, find and edit the desired output in the report.

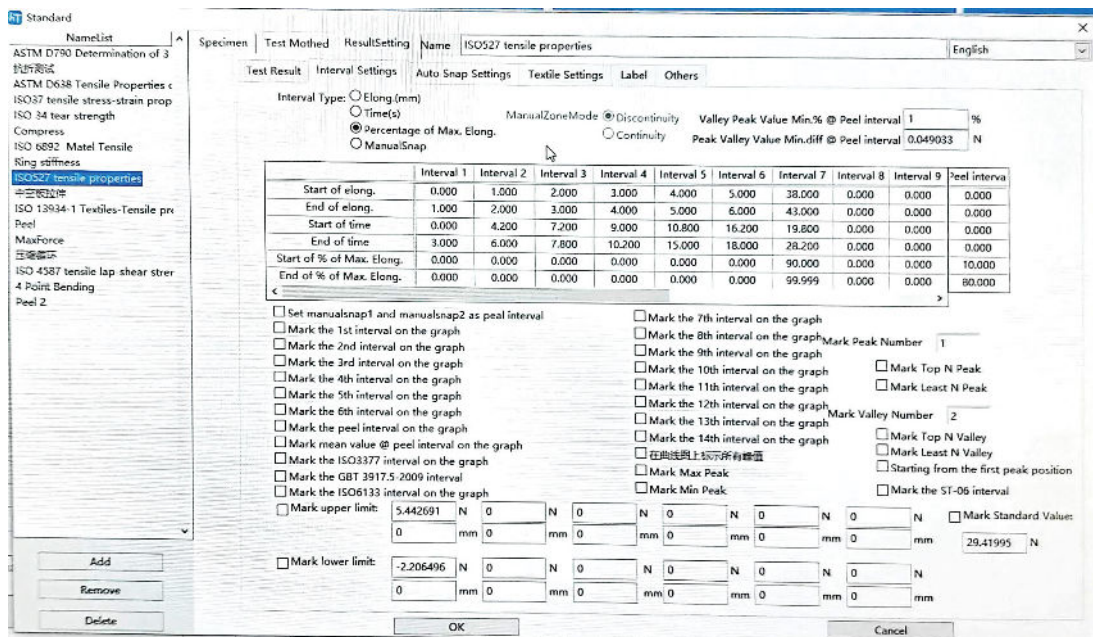


- Interval setting interface: the main functions include the selection of interval mode, the display of curve marking force, manual selection of the desired stripping interval, and the peak-to-valley ratio and minimum drop force of the stripping interval.

Software Interface

Results Setting Screen

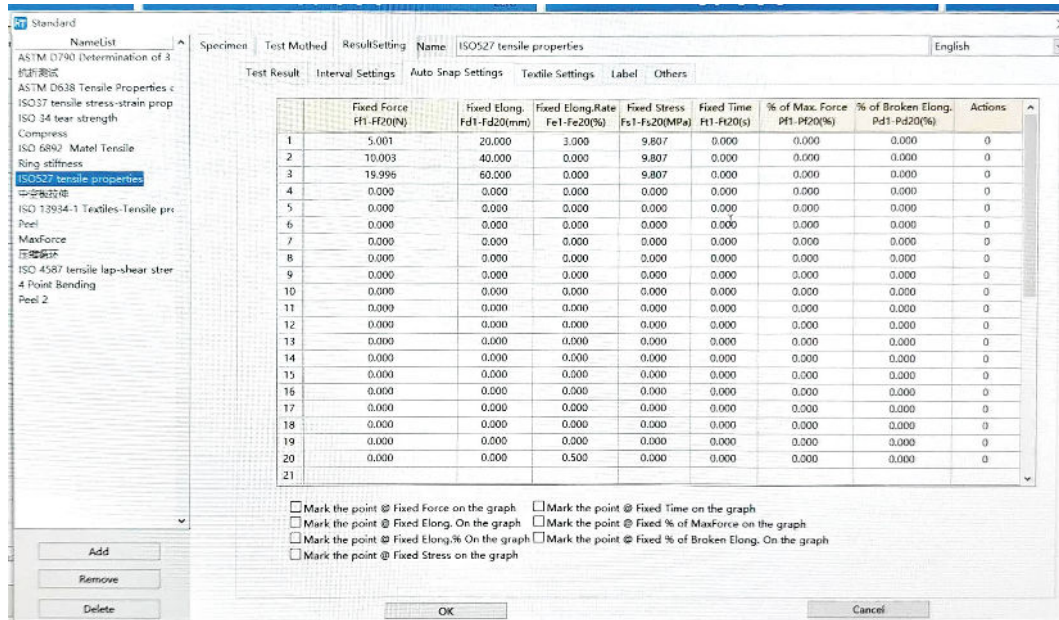

- Auto Picking Points Setting Interface: The main functions include auto picking points setting and supporting picking points on the back and forth curves. An action of 0 indicates that points are taken on the whole curve. An action of 1 indicates that the point is taken at the first test step.

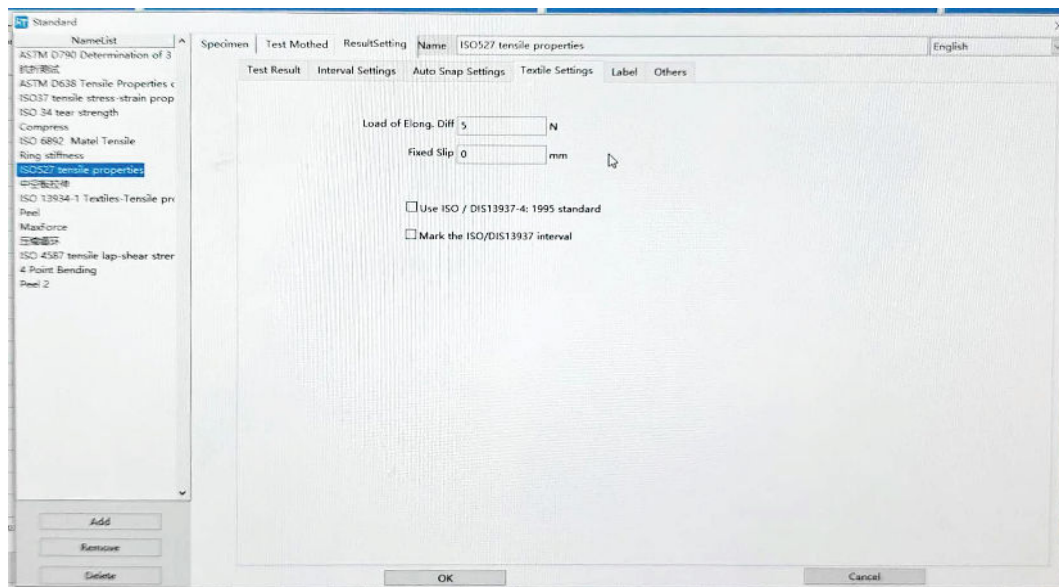

- Textile test setup interface: the main functions include 1) elongation difference load: calculating the setup parameters of elongation difference; 2) specified slip: calculating the setup parameters of slip resistance.


Software Interface

Multi-image Interface



- Force-deformation, force-time deformation, and deformation-time graphs can be observed.

Multi-image Interface

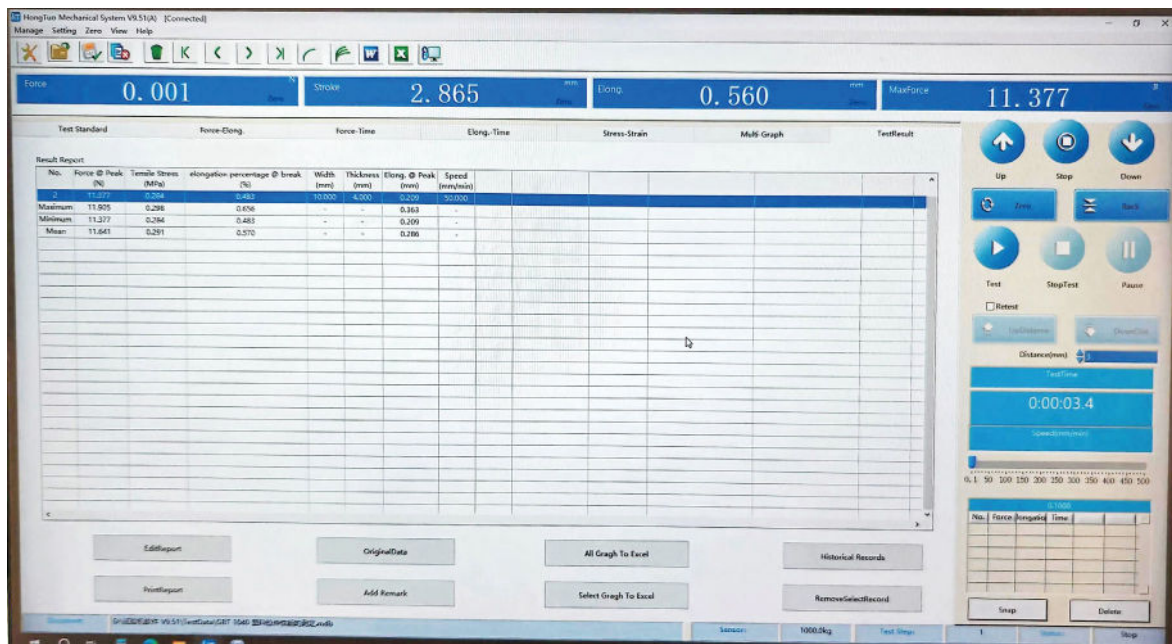

- Edit report, print report, output original data to excel, add note information, output all curves to excel, output selected curves to excel, view historical data, remove selected records.







Technical Specification

Model		UTM-DCH								
Subdivision Model		UTM-DCH-5	UTM-DCH-10	UTM-DCH-20	UTM-DCH-50	UTM-DCH-100	UTM-DCH-200	UTM-DCH-500	UTM-DCH-1000	UTM-DCH-2000
	KN	0.05	0.1	0.2	0.5	1	2	5	10	20
Capacity	KG	5	10	20	50	100	200	500	1000	2000
	lb	11	22	44	110	220	440	1102	2204	4408
Unit Switching		G,Kg,Ib,N,KN								
Displacement Unit Switching		Inch/cm/mm								
Testing Machine Class		Class 0.5								
Effective Force Measurement Range		0.4%~100%FS								
Force Accuracy		Within +0.5% of the indicated value								
Force Value Resolution		1/500000								
Displacement Resolution		≤0.05um								
Displacement Accuracy		Within 10.5% of the indicated value								
Deformation Measuring Range		0.2%~100%FS								

Technical Specification

Precision of Deformation Indication	Within +0.5% of the indicated value
Limit of Large Deformation Indication Error	Within +0.5% of the indicated value (optional)
Maximum Test Speed	500mm/min;1000mm/min(optional)The maximum value is 1000mm/min(optional)
Minimum Test Speed	0.01mm/min
Speed Accuracy	Within 1% of the indicated value
Measuring Width	Test stroke without fixture: 1330mm; Test stroke with fixture:800mm
Effective Width	420mm,650mm(optional)
Fixture Configuration	A group of tensile fixtures
Return Mode	Manual or automatic options, automatic return after the end of the test or manual return to the initial position
Stop Method	1.The maximum breaking value of automatic stop2.The upper and lower limits of safety setting stop
Safety Device	1.Mechanical stroke switch protection2.Emergency stop switch emergency braking
Overload Protection	Over 10% of the maximum load, the machine automatically protects
Power Supply	220v.AC/50HZ; (110v.AC/60HZ can be selected by country)
Weight	Net Weight: about 185KG; Gross Weight: about 220KG
Dimension	Mainframe:L*W*H:800mm*550mm*1700mm Package:L* W*H:900mm*650mm*1800mm

Standard Delivery

Name	Qty	Photo
Machine Mainframe	1pc	
Power Cord	1pc	/
Test Software Program CD 1	1pc	/
Data Cable	1pc	/
Fixture	1pc	
Computer	1pc	
Printer	1pc	
Instruction Manual	1copy	
Product Certificate/Warranty	each 1copy	

Optional Delivery

Optional

Small Deformation Metal Extensometer

Large Deformation Extensometer(1000mm,0.01mm)

Other Fixtures

Mikrosize Precision Instrument Co.,Ltd

Add: A-4035 RuiFeng Business Expo , Wuhu City, China , 241000.

Tel: 0553-2836939 Fax:0553-2836938 Web: www.mikrosize.com

